


Certificate of Factory Calibration

1/4" IEPE Free Field Measurement Microphone

Type : MI19 J

Serial No. : 1016

Sensitivity : 51.0 mV/Pa (@ 1 kHz | 23°C | 1019 hPa)

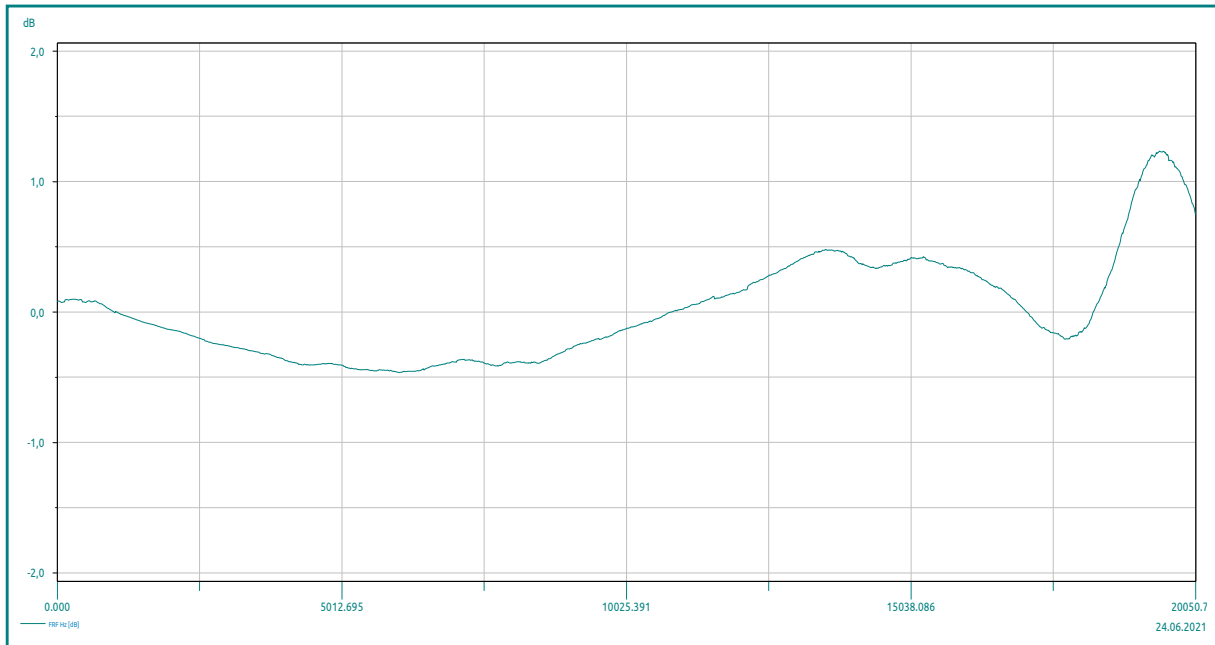

BSWA Full Frequency Coupler CA916 # 540002

Reference Microphone # MPA231

Svantek SV30A # 14126

Plug.n.DAQ Lite # 353

Software : DASyLab Pro 2020.1

Calibrated by

Rogá

