


Certificate of Factory Calibration

1/2" Measurement Microphone Capsule - Prepolarizrd - Class 1

Type : AWA 1425

Serial No. : H- 38081

Sensitivity : 41.4 mV/Pa (@ 1 kHz | 22°C | 1014 hPa)

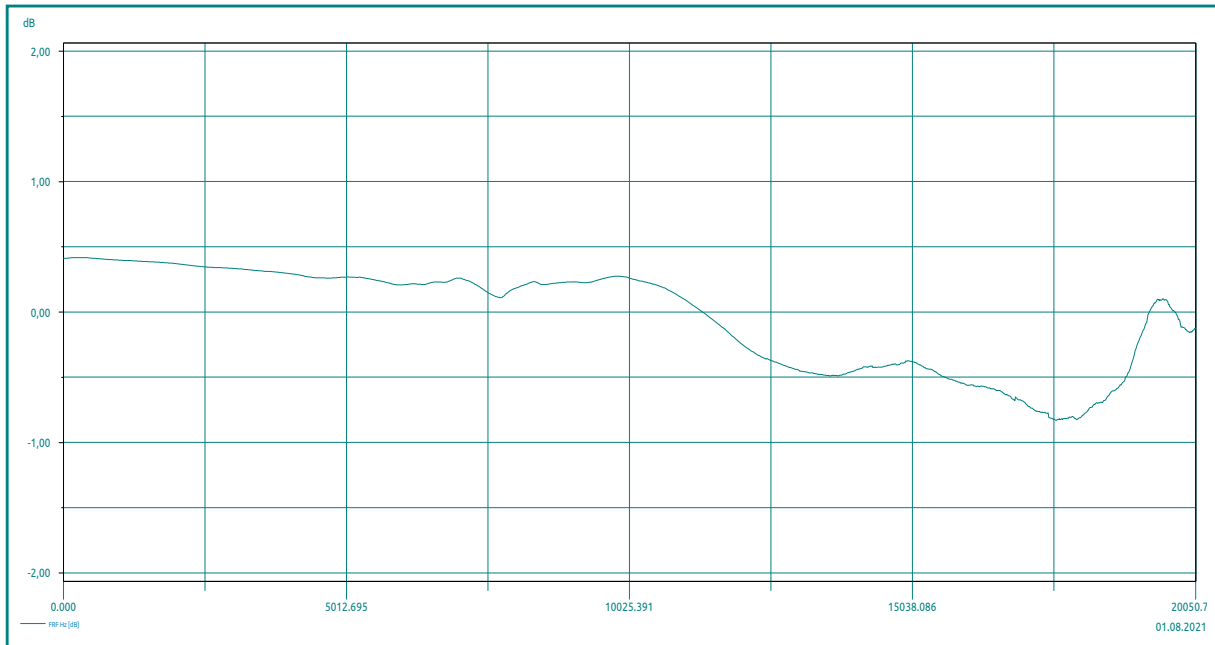

BSWA Full Frequency Coupler CA916 # 540002

Reference Microphone # MPA231

Svantek SV30A # 14126

Plug.n.DAQ Lite # 353

Software : DASyLab Pro 2020.1

Calibrated by

Rogá

