


Certificate of Factory Calibration

1/4" IEPE Free Field Measurement Microphone

Type : MI15
Serial No. : 890
Sensitivity : 50.0 mV/Pa (@ 1 kHz | 23 °C | 1010 hPa)

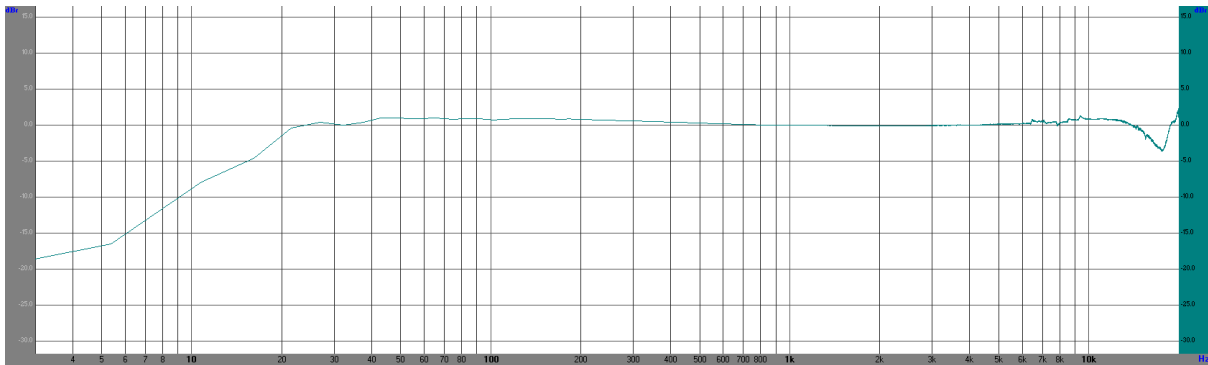

BSWA Full Frequency Coupler CA916
Reference Microphone
Svantek SV30A
Plug.n.DAQ Lite
Software
Measurement uncertainty

540002
MPA231
14126
353
Visual Analyzer v 2021R1 32 bits
0.20 dB

Calibrated by, 5/12/2022


Romuald Gawlik
CEO and Founder

